


Journal Pre-proof

Biosensing detection of the SARS-CoV-2 D614G mutation

Yang Zhang, Hui Xi, Mario Juhas

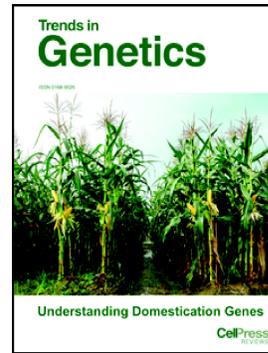

PII: S0168-9525(20)30334-6

DOI: <https://doi.org/10.1016/j.tig.2020.12.004>

Reference: TIGS 1772

To appear in: *Trends in Genetics*

Please cite this article as: Y. Zhang, H. Xi and M. Juhas, Biosensing detection of the SARS-CoV-2 D614G mutation, *Trends in Genetics* (2020), <https://doi.org/10.1016/j.tig.2020.12.004>

This is a PDF file of an article that has undergone enhancements after acceptance, such as the addition of a cover page and metadata, and formatting for readability, but it is not yet the definitive version of record. This version will undergo additional copyediting, typesetting and review before it is published in its final form, but we are providing this version to give early visibility of the article. Please note that, during the production process, errors may be discovered which could affect the content, and all legal disclaimers that apply to the journal pertain.

© 2020 Published by Elsevier.

## Biosensing detection of the SARS-CoV-2 D614G mutation

Yang Zhang<sup>1\*</sup>, Hui Xi<sup>1</sup>, Mario Juhas<sup>2</sup>

<sup>1</sup>College of Science, Harbin Institute of Technology (Shenzhen), Shenzhen, Guangdong, 518055, China.

<sup>2</sup>Medical and Molecular Microbiology Unit, Department of Medicine, Faculty of Science and Medicine, University of Fribourg, Fribourg, Switzerland.

\* Correspondence: zhangyang07@hit.edu.cn (Y. Zhang)

**Abstract:** The emergence of a SARS-CoV-2 mutant virus with an amino acid change from aspartate to a glycine residue at position 614 (D614G) has been reported and this mutant appears to be now dominant in the pandemic. Efficient detection of the SARS-CoV-2 D614G mutant by biosensing technologies is therefore crucial for the control of the pandemic.

**Keywords:** Spike; Loop-mediated isothermal amplification (LAMP); Restriction endonucleases; CRISPR-Cas; Nanopore; Hybridization

### **D614G mutation increases SARS-CoV-2 infectivity**

The COVID-19 pandemic, caused by the severe acute respiratory syndrome coronavirus 2 (SARS-CoV-2), has rapidly escalated into the largest global public health emergency of the past decades. As of December , 2020, more than 75 million people have been infected and more than 1.7 million have died as a result of the SARS-CoV-2 infection <sup>i</sup>. SARS-CoV-2 shares similarities with two other beta coronaviruses, causing serious and potentially deadly respiratory tract infections, SARS-CoV and Middle East respiratory syndrome coronavirus (MERS-CoV). The open reading frames (ORFs) of approximately 30 kb SARS-CoV-2 genome encode 16 nonstructural and 4 structural proteins, namely Envelope (E), Membrane (M), Nucleocapsid (N) and Spike (S) (Figure 1A) [1].

The sequencing of thousands of SARS-CoV-2 genomes revealed a number of recurrent mutations, out of which an amino acid change from aspartate to a glycine residue at position 614 (D614G) in spike protein has gained the most attention. D614G is a missense mutation where the amino acid change is caused by an A-to-G nucleotide mutation at genomic position 23403 [2]. D614G mutation has been identified by phylogenetic analysis of over a thousand of SARS-CoV-2 genomes. While D614G mutation was relatively rare at the onset of pandemic, by June 2020 this mutation was found in the majority of COVID-19 patients [1-3]. D614G point mutation is predominant amongst the SARS-CoV-2 genomes currently circulating in the population [2]. Furthermore, D614G mutation is located in the S1 subunit of the spike protein which is crucial for the entry of the SARS-CoV-2 virus into the host cell (Figure 1B, C). The spike protein of SARS-CoV-2 is cleaved into S1 and S2 subunits by host proteases, with the S1 domain responsible for receptor binding and the S2 domain mediating membrane fusion [1, 4]. The receptor binding domain (RBD) within the S1 subunit of spike protein interacts with the

angiotensin-converting enzyme 2 (ACE2) receptor on the surface of the host cells, thus mediating virus entry [1, 2]. Although, the D614G point mutation is outside of the RBD (Figure 1C), it has been suggested to have an impact on the infectivity of the virus. The rapid spread of the D614G mutant version of the virus was hypothesized to correlate with the higher infectivity of SARS-CoV-2 harboring this mutation [2, 4]. Clinical samples from patients infected with D614G mutant were shown to have higher viral RNA levels and higher pseudovirus titers [2]. Due to the widespread and impact of the D614G mutation on SARS-CoV-2 biology, novel methods for its fast and reliable detection are of the highest importance.

### **Biosensing technologies for the detection of SARS-CoV-2 D614G mutation at protein level**

Development of biosensing technologies for the efficient and rapid detection of SARS-CoV-2 and its D614G mutation is crucial for the control of the pandemic. One such promising method, surface plasmon resonance (SPR), has been used to investigate the effect of D614G mutation on the binding kinetics of SARS-CoV-2 spike protein with human ACE2 [5]. The binding rates of spike protein with and without D614G mutation were similar, but the dissociation rate of D614G mutant was faster, which contributes to the decrease in binding affinity [5]. This observation could be exploited for the engineering of a SPR-based biosensing platform employing ACE2 protein for SARS-CoV-2 D614G mutant protein detection (Figure 2A). Alternatively, biosensing based on aptamers, antibodies or nanobodies can be designed to distinguish the spike protein with or without D614G mutation (Figure 2A). Aptamers are short single-stranded nucleic acid sequences which fold into tertiary structures to bind any desired target [6]. Similar to antibodies, aptamers have also been used in the Enzyme-linked Immunosorbent Assay (ELISA) and colloidal gold immunochromatographic strips for the detection of N protein of SARS-CoV-2 [7].

In addition to antibodies, nanobodies derived from the VHH domain of single-heavy-chain antibodies have also been raised with high affinity for the spike protein of SARS-CoV-2 [8, 9].

Aptamers, antibodies, and nanobodies specifically distinguishing D614G mutation within the spike protein, can be used as biorecognition elements, and then incorporated into the ELISA and lateral flow assays (Figure 2A).

Although the serological assay is rapid and requires minimal equipment, its efficacy is limited due to the presence of low amounts of the viral protein or antigen in the blood of patients. Furthermore, current studies suggest that the D614G mutation retains similar sensitivity to antibodies that target the receptor binding domain [5]. Thus, the possibility of reliable detection of mutation-specific antibodies by D614G and D614 antigens will require further investigation. Overall, despite the need for the conversion of an RNA single stranded genome of SARS-CoV-2 into cDNA for detection purposes, biosensing technologies aimed at the detection of D614G mutation at the gene level show much greater promise.

### **Biosensing technologies for the detection of SARS-CoV-2 D614G mutation at gene level**

DNA sequencing and polymerase chain reaction (PCR) are current standard tests for detecting the presence of SARS-CoV-2. In conjunction with DNA sequencing and different types of PCR-based techniques, capillary electrophoresis, surface-enhanced Raman spectroscopy (SERS), mass spectrometry (MS) and denaturing high performance liquid chromatography (dHPLC) [10-12] can also be used to screen for the presence of the D614G mutation. However, these conventional methods are often complex, tedious and time consuming. Novel biosensing technologies for rapid monitoring of D614G are therefore urgently needed.

Loop-mediated isothermal amplification (LAMP) is a PCR based method for the amplification of nucleic acids under isothermal conditions, which does not require a thermal cycler or expensive reagents. LAMP has been successfully applied for the rapid (as little as 30 min) and colorimetric detection of SARS-CoV-2 [13]. A set of primers can be designed and optimized to specially distinguish the D614G mutant genotype. LAMP is fast, and its products can be detected with electrochemical and optical readouts, or even by the naked eye, making it suitable for point-of-care testing (POCT) of SARS-CoV-2 D614G mutation (Figure 2A).

D614G mutation corresponds to the alteration of an adenine to a guanine at genomic position 23403 (Figure 1C) [2]. Consequently, D614G mutation can be detected using restriction endonucleases to enzymatically cleave deoxynucleotides at this specific site, following double stranded cDNA synthesis. In this case, restriction endonucleases FokI, BtsCI, BseGI and BstF5I can be used for specific recognition and cleaving of the GGATG sequence in the wild-type D614, while leaving the mutant G614 sequence intact. The specific cleaving of the point mutation can be combined with suitable signal amplification strategies, such as rolling circle amplification (RCA), strand displacement amplification (SDA) and isothermal exponential amplification (EXPAR) [14] for the optical and electrochemical detection of the D614G mutant version (Figure 2B).

Besides restriction endonucleases, RNA-guided Cas endonucleases that catalyze site-specific cleavage of DNA can also be used to detect point mutations [15]. For example, a CRISPR–Cas12-based assay was combined with LAMP for rapid (less than 40 min) and accurate detection of SARS-CoV-2 in clinical samples. Followed by Cas12 detection of viral sequences, visualization was achieved using FAM-biotin reporter molecule and lateral flow strips [16]. Similar CRISPR/Cas systems can be exploited for the accurate and scalable detection of SARS-

CoV-2 D614G mutation on a lateral flow strip using different signal readout based on electrochemical and optical techniques (Figure 2B).

Besides using endonucleases for the mutation site recognition, engineered pore-forming proteins could be applied directly to gene sequencing and D614G mutant detection. Nanopore sequencing technologies constitute a versatile platform for DNA/ RNA sequencing and have been also used for real-time sequencing of the SARS-CoV-2 genome [17, 18]. Nanopore sequencing directly measures changes in currents generated when DNA/RNA strands pass through the nanopore. The electrical signal corresponding to each nucleic acid can be recorded in real-time and used for subsequent sequence analysis. Although nanopore sequencing offers high throughput and accurate genotyping of SARS-CoV-2 [14], it is significantly slower, taking hours to obtain testing results (Figure 2B).

Hybridization-based biosensing platforms are highly specific and represent a promising tool for nucleic acid and single-nucleotide mutation detection. SARS-CoV-2 RNA was detected on formalin-fixed paraffin-embedded (FFPE) tissue from COVID-19 autopsies by *in situ* hybridization (ISH) [19]. Moreover, an amplification-free immunoassay was developed for the fluorescence detection of SARS-CoV-2 RNA in the throat swab or sputum sample. The assay is implemented on a lateral flow strip based on hybridization of viral RNA with DNA probes and selective capture of RNA-DNA hybrids by monoclonal antibodies [20]. Hybridization techniques using point-mutated probes and corresponding perfect matching probes can be also confidently employed for the D614G mutation detection. To scale from small sample numbers to thousands, microarray hybridization analysis is the most appropriate technology, employing tens to hundreds of probes for single base mismatch discrimination (Figure 2B).

Considered the incredible demand for SARS-CoV-2 genotyping, a number of different biosensing techniques with various biorecognition elements and detection principles from diverse industry sources are needed to address the immediate shortage of reliable and efficient tests in the face of the global COVID-19 pandemic.

### **Acknowledgements**

The work was supported by the Natural Science Foundation of Shenzhen City (Project number JCYJ20180306172131515).

### **Resources:**

- i) <https://www.who.int/emergencies/diseases/novel-coronavirus-2019/situation-reports/>

**References**


1. Dearlove, B. et al. (2020) A SARS-CoV-2 vaccine candidate would likely match all currently circulating variants. *Proc. Natl. Acad. Sci. U S A* 117, 23652-23662.
2. Korber, B. et al. (2020) Tracking Changes in SARS-CoV-2 Spike: Evidence that D614G Increases Infectivity of the COVID-19 Virus. *Cell* 182, 812-827.
3. Isabel, S et al (2020) Evolutionary and structural analyses of SARS-CoV-2 D614G spike protein mutation now documented worldwide. *Sci Rep* 10, 14031.
4. Li, Q. et al. (2020) The Impact of Mutations in SARS-CoV-2 Spike on Viral Infectivity and Antigenicity. *Cell* 182, 1284-1294.
5. Yurkovetskiy, L. et al. (2020) Structural and Functional Analysis of the D614G SARS-CoV-2 Spike Protein Variant. *Cell* 183, 733-751.
6. Zhang, Y. et al. (2019) Recent Advances in Aptamer Discovery and Applications. *Molecules* 24, 941.
7. Zhang, L. et al. (2020) Discovery of sandwich type COVID-19 nucleocapsid protein DNA aptamers. *Chem Commun* 56, 10235-10238.
8. Schoof, M. et al. (2020) An ultrapotent synthetic nanobody neutralizes SARS-CoV-2 by stabilizing inactive Spike. *Science*, DOI: 10.1126/science.abe3255.
9. Huo, J. et al. (2020) Neutralizing nanobodies bind SARS-CoV-2 spike RBD and block interaction with ACE2. *Nat Struct Mol Biol* 27, 846-854.
10. Li, Y. et al. (2019) Direct approach toward label-free DNA detection by surface-enhanced raman spectroscopy: Discrimination of a single-base mutation in 50 base-paired double helices. *Anal Chem* 91, 7980-7984.

11. Mosko, M. et al. (2016) Ultrasensitive detection of multiplexed somatic mutations using MALDI-TOF mass spectrometry. *J Mol Diagn* 18, 23-31.
12. Liu, X. et al. (2020) Detection of mutant genes with different types of biosensor methods. *Trends Analyt Chem* 126, 115860.
13. Rabe, B.A. and Cepko, C. (2020) SARS-CoV-2 detection using isothermal amplification and a rapid, inexpensive protocol for sample inactivation and purification. *Proc. Natl. Acad. Sci. U S A* 117, 24450-24458.
14. Mittal, S. et al. (2019) Bio-analytical applications of nicking endonucleases assisted signal-amplification strategies for detection of cancer biomarkers-DNA methyl transferase and microRNA. *Biosens Bioelectron* 124, 233-243.
15. Gootenberg, J.S. et al. (2017) Nucleic acid detection with CRISPR-Cas13a/C2c2. *Science* 356, 438-442.
16. Broughton, J.P. et al. (2020) CRISPR-Cas12-based detection of SARS-CoV-2. *Nat. Biotechnol.* 38, 870-874.
17. Wang, M. et al. (2020) Nanopore Targeted Sequencing for the Accurate and Comprehensive Detection of SARS-CoV-2 and Other Respiratory Viruses. *Small* 16, e2002169.
18. Liu, L. and Wu, H.C. (2016) DNA-Based Nanopore Sensing. *Angew. Chem. Int. Ed. Engl.* 55, 15216-15222.
19. Massoth, L.R. et al. (2020) Comparison of RNA In Situ Hybridization and Immunohistochemistry Techniques for the Detection and Localization of SARS-CoV-2 in Human Tissues. *Am. J. Surg. Pathol.* DOI: 10.1097/PAS.0000000000001563

20. Wang, D. et al. (2020) Rapid lateral flow immunoassay for fluorescence detection of SARS-CoV-2 RNA. *Nat Biomed Eng* 4, 1150-1158.


Journal Pre-proof

## Figure legends

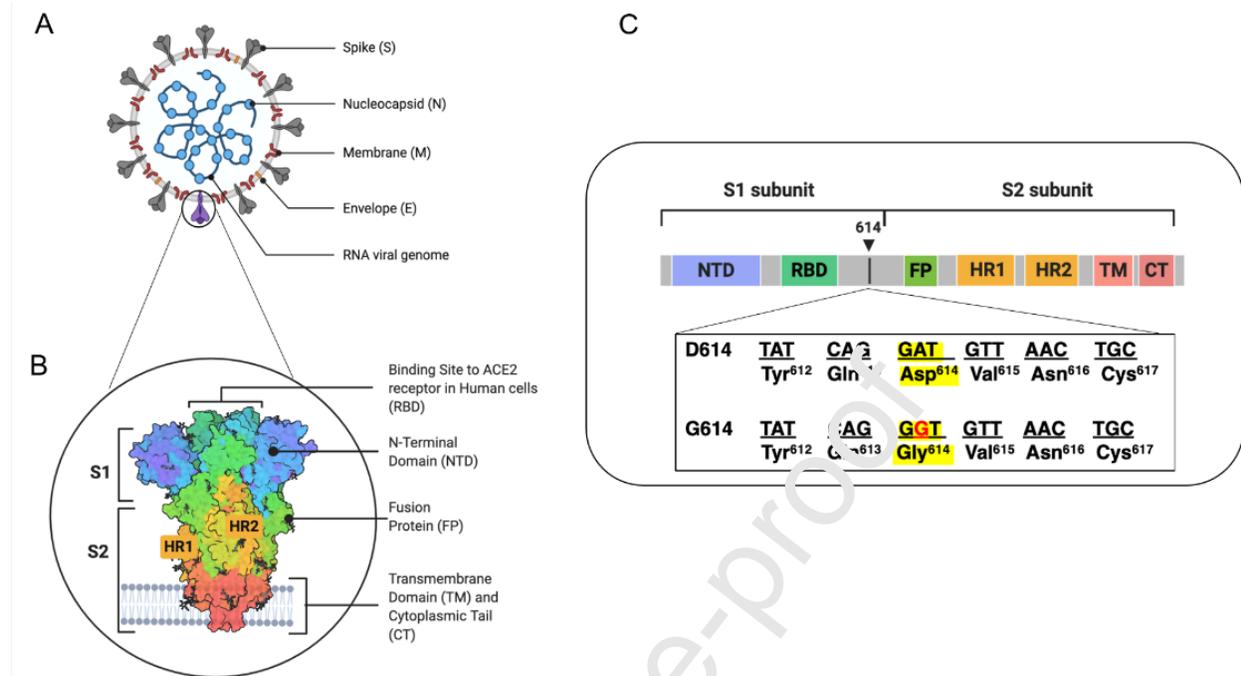

**Figure 1. D614G mutation in SARS-CoV-2 spike protein.**

(a) The structure of SARS-CoV-2 includes the surface spike (S) protein, the nucleocapsid (N) protein, the membrane (M) protein, the envelope (E) protein and the RNA genome. (b) Crystal structure of SARS-CoV-2 spike (S) protein. PDB ID: 6VXX. (c) Schematic representation of the SARS-CoV-2 spike protein (S). Abbreviations: S1, S1 subunit; S2, S2 subunit; NTD, N-terminal domain; RBD, receptor binding domain; FP; fusion protein; HR1/2, heptad repeat 1/2; TM, transmembrane domain; and CT, cytoplasmic tail. Figure was created in part with BioRender.

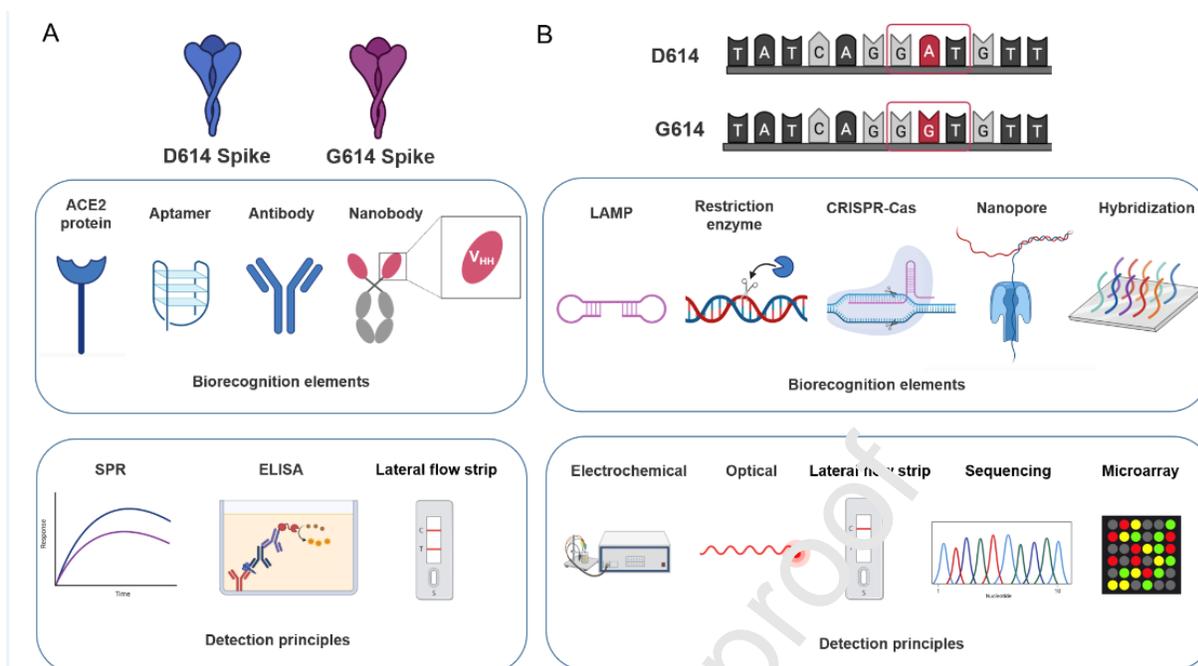

**Figure 2. Biosensing technologies for the detection of D614G mutation.**

(a) Detection of D614G mutation at the protein level. D614G mutation at the protein level can be identified using ACE2 protein, aptamers, antibodies or nanobodies. Signal generated by these biorecognition elements can be detected by different detection principles, such as surface plasmon resonance (SPR), Enzyme-linked Immunosorbent Assay (ELISA), and lateral flow strips. (b) Detection of D614G mutation at the gene level. D614G mutation in SARS-CoV-2 spike protein corresponds to the alteration of an adenine to a guanine at genomic position 23403. Promising approaches for the recognition of the D614G mutation at the gene level include LAMP, restriction enzymes, CRISPR-Cas, nanopore and oligo probe hybridization. Specific signal generated by these biorecognition techniques can be then used for the detection of D614G mutation using variety of detection principles, such as electrochemical and optical techniques, lateral flow strips, sequencing or microarrays. Figure was created in part with BioRender.